



Calibration: polynomial order = 3

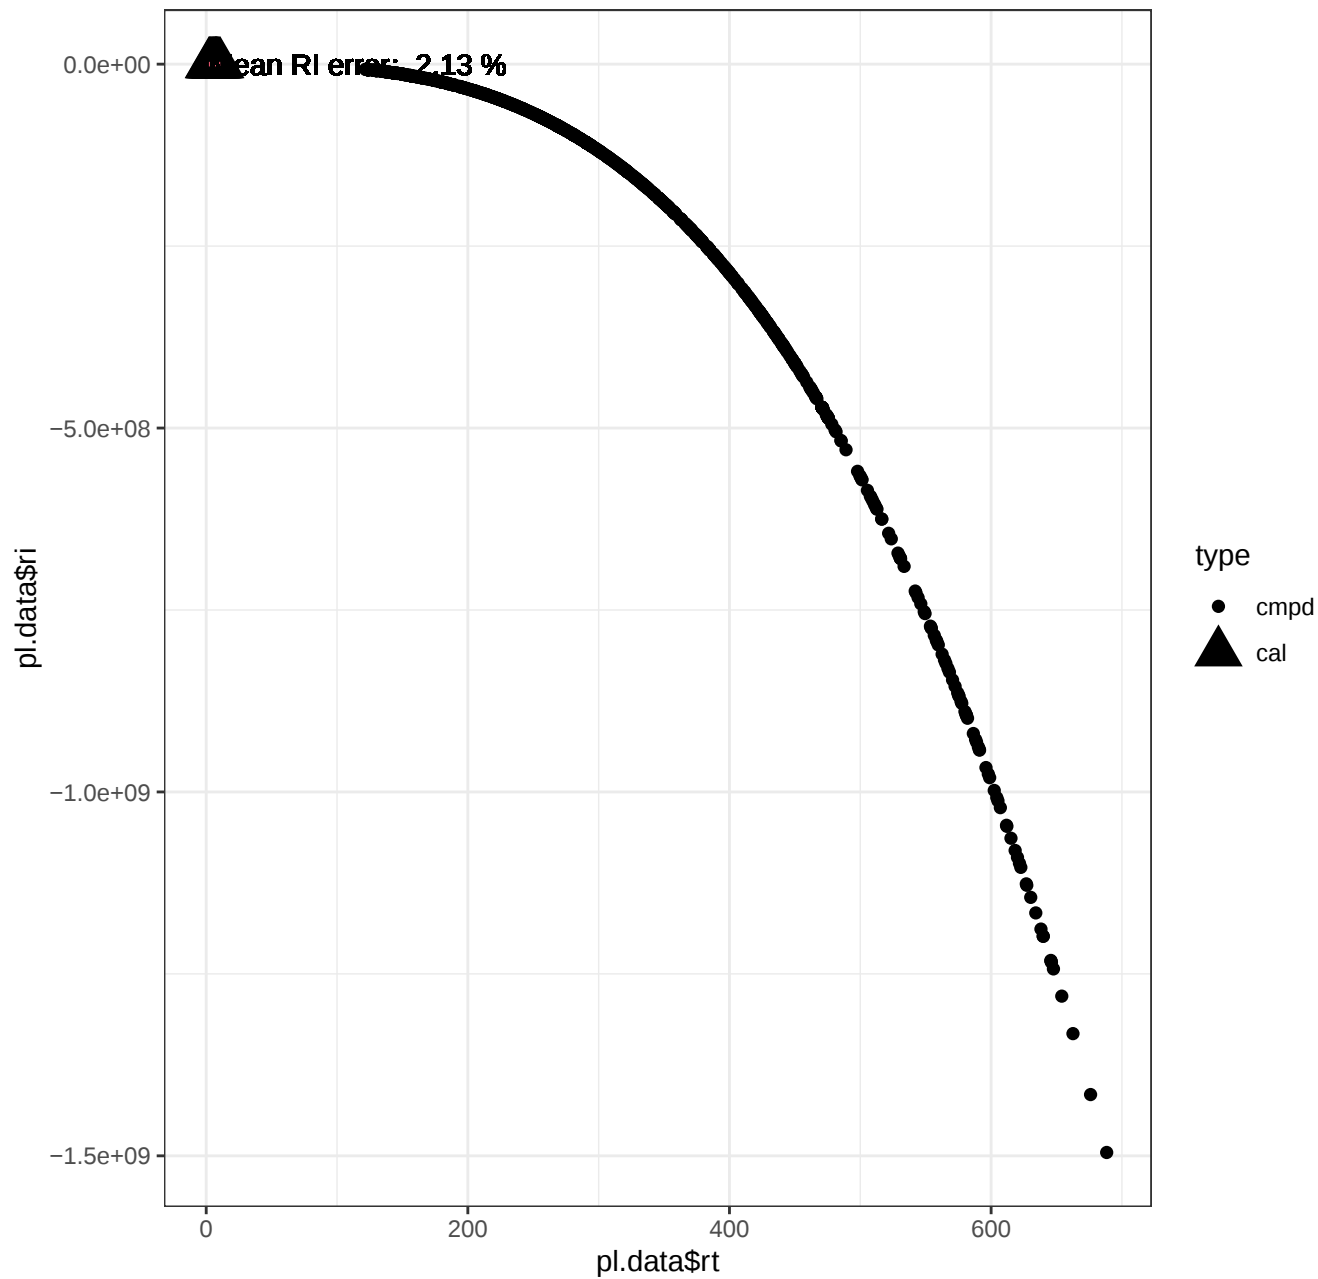


MSdata

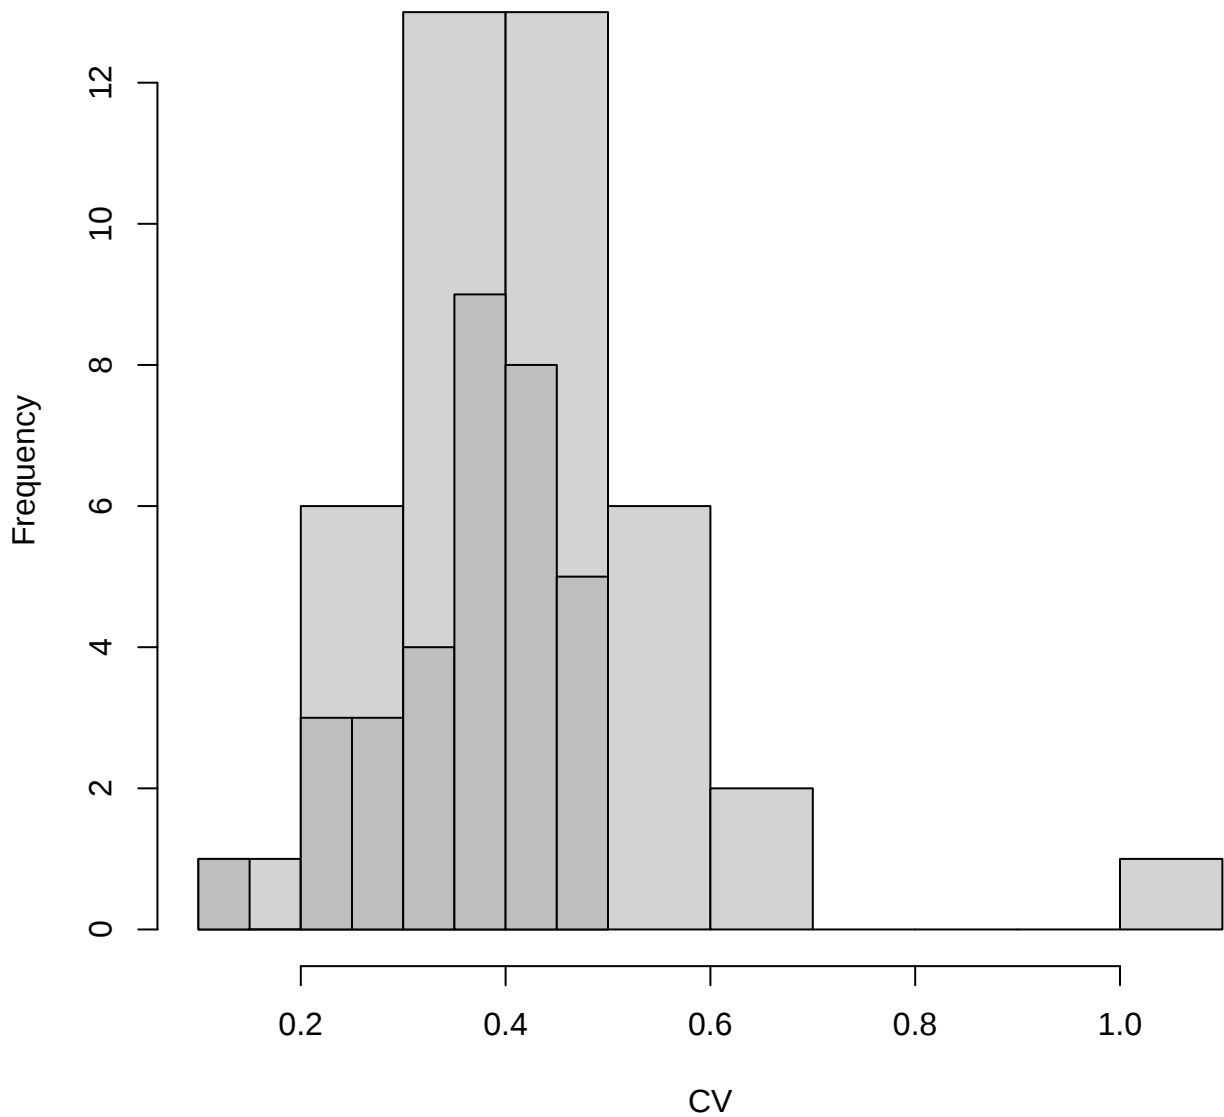

histogram of MSdata CVs from QC samples

20% quantiles in red on top axis

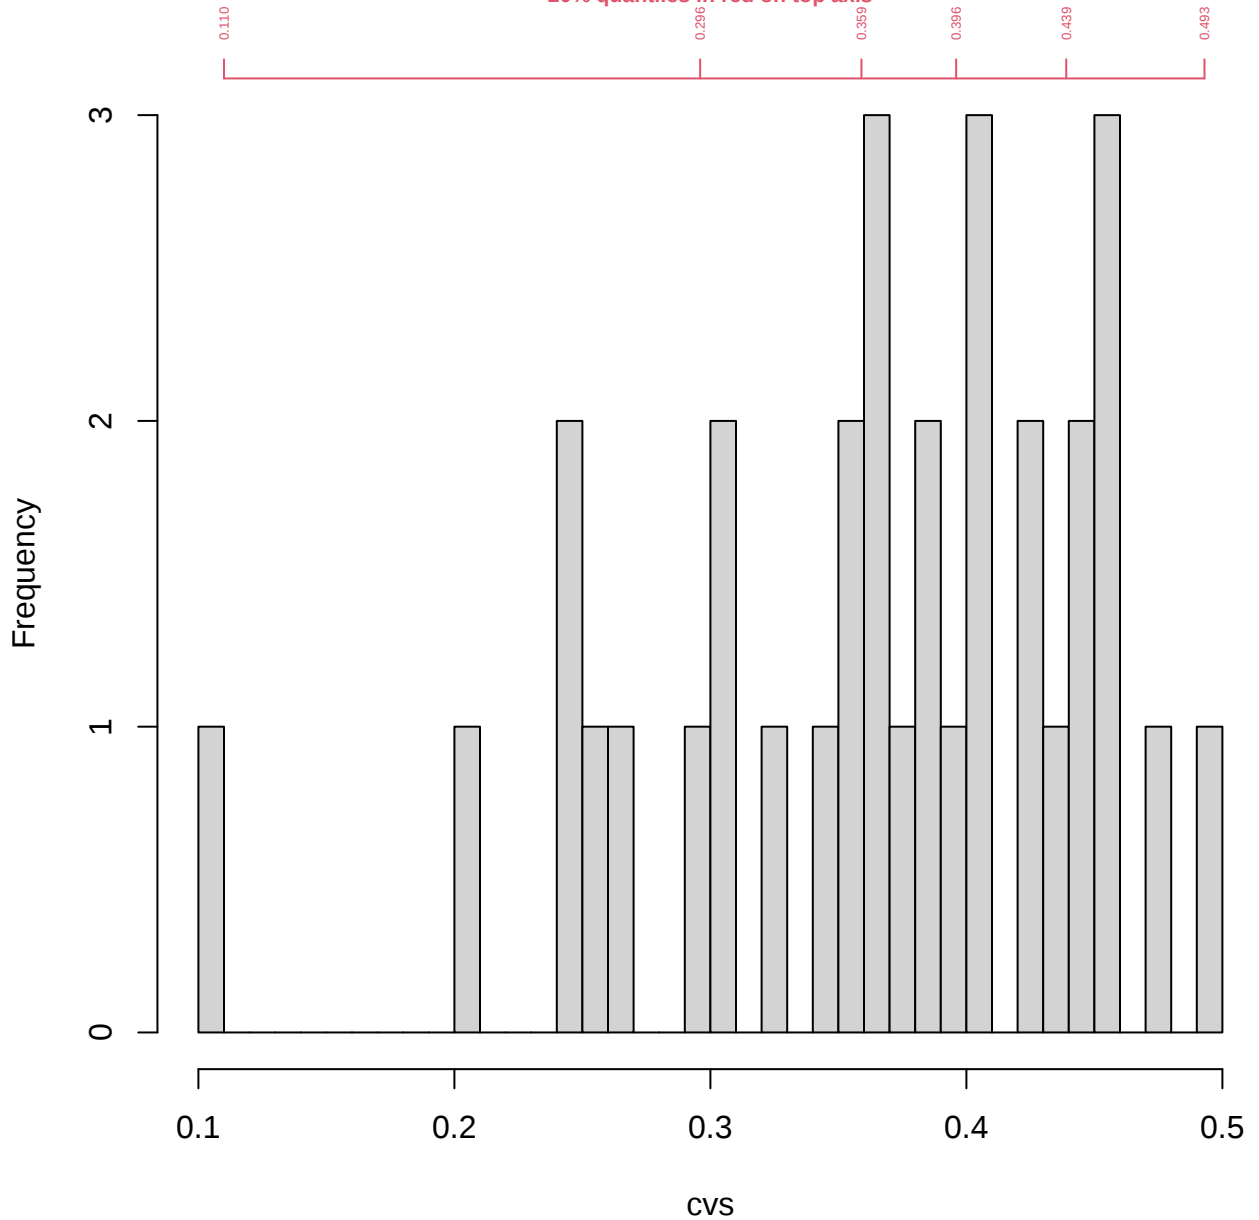

histogram of SpecAbund CVs from QC samples

20% quantiles in red on top axis

Frequency

1

0

0.334

0.357

0.378

0.394

0.414

0.438

0.34

0.36


0.38

0.40


0.42

0.44

CVS

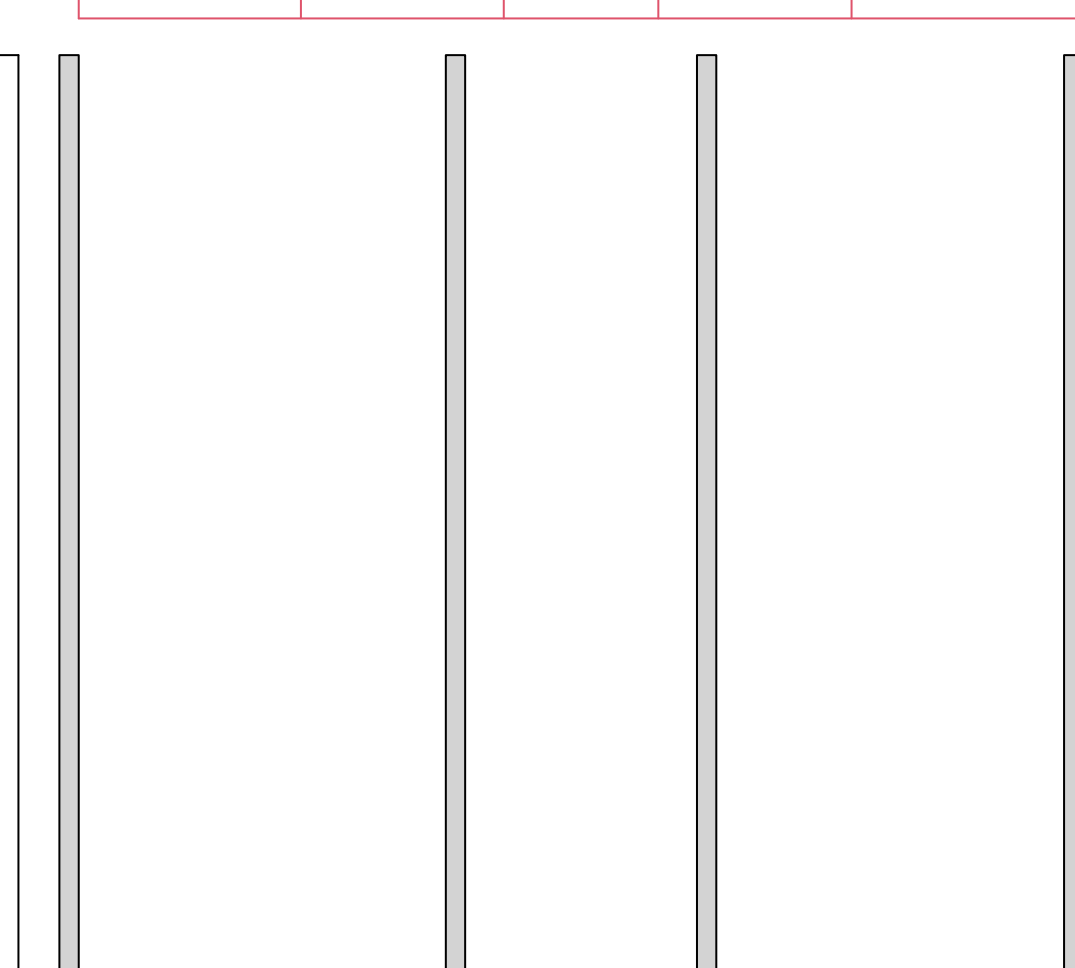


MSdata

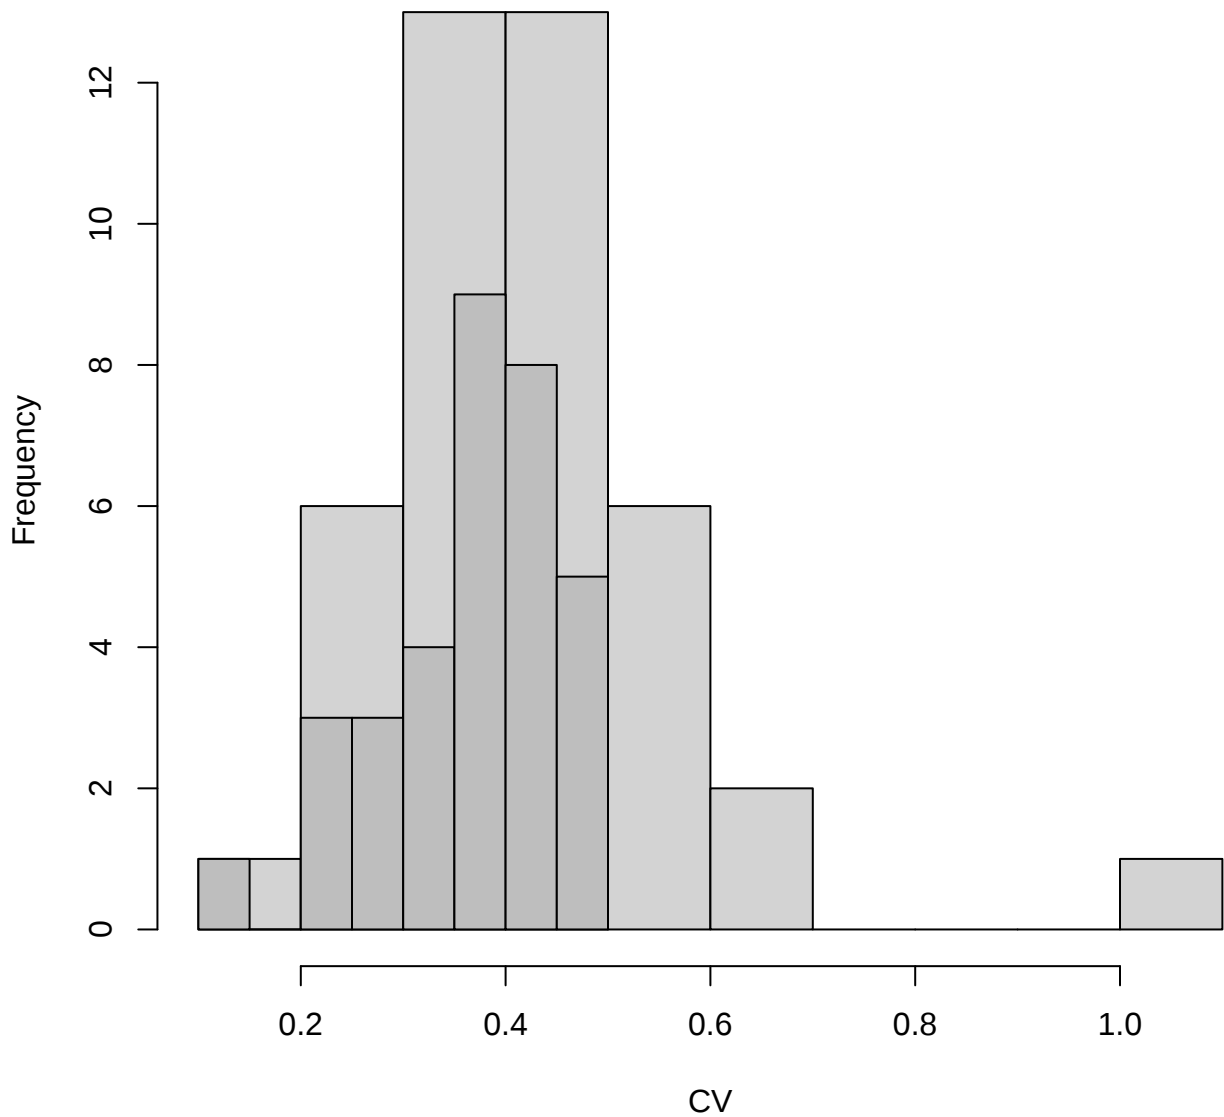

histogram of MSdata CVs from QC samples

20% quantiles in red on top axis

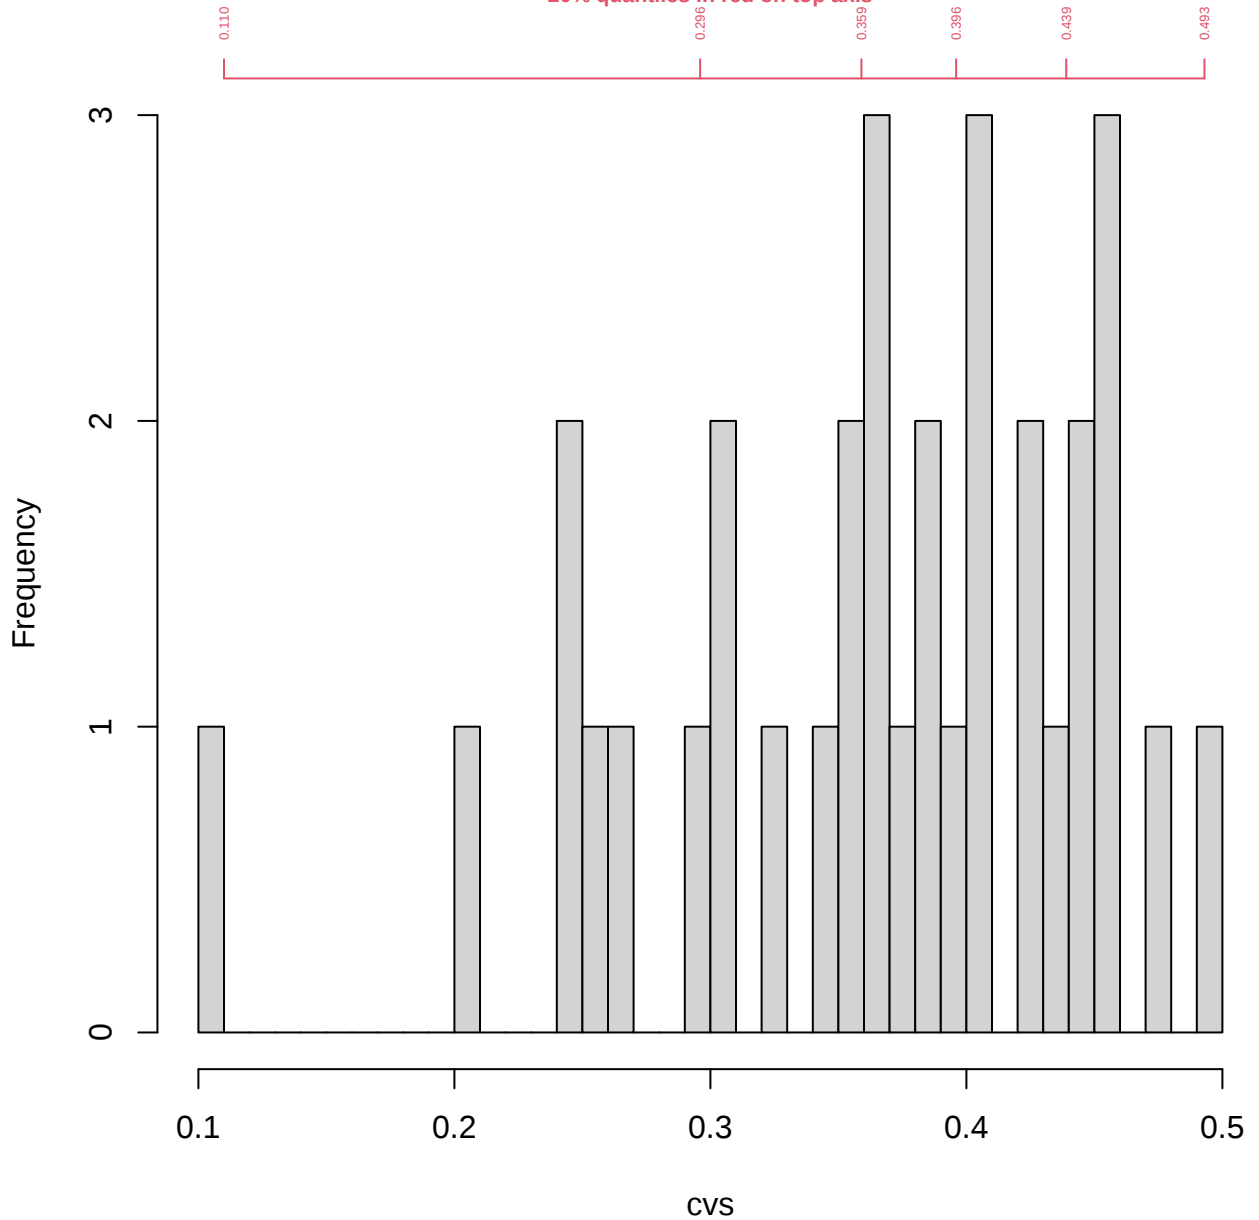

histogram of SpecAbund CVs from QC samples

20% quantiles in red on top axis

Frequency

1

0

0.334

0.357

0.378

0.394

0.414

0.438

0.34

0.36

0.38

0.40

0.42

0.44

CVS

